




## Adipotide HPLC Purity Test Report

Product Name : Adipotide ( CKGGRAKDC-GG-D(KLAKLAK) 2)  
Batch No. : P170919ADI  
Column : Xbridge BEH130 C18, 4.6\*250mm, 5um  
Solvent A : 0.1%Trifluoroacetic in 100% Acetonitrile  
Solvent B : 0.1%Trifluoroacetic in 100% Water  
Gradient :  
          A                  B  
0.0min 23%                  77%  
25.0min 48%                  52%  
25.1min 100%                 0%  
30.0min                      Stop  
Flow rate : 1.0ml/min  
Wavelength : 220nm

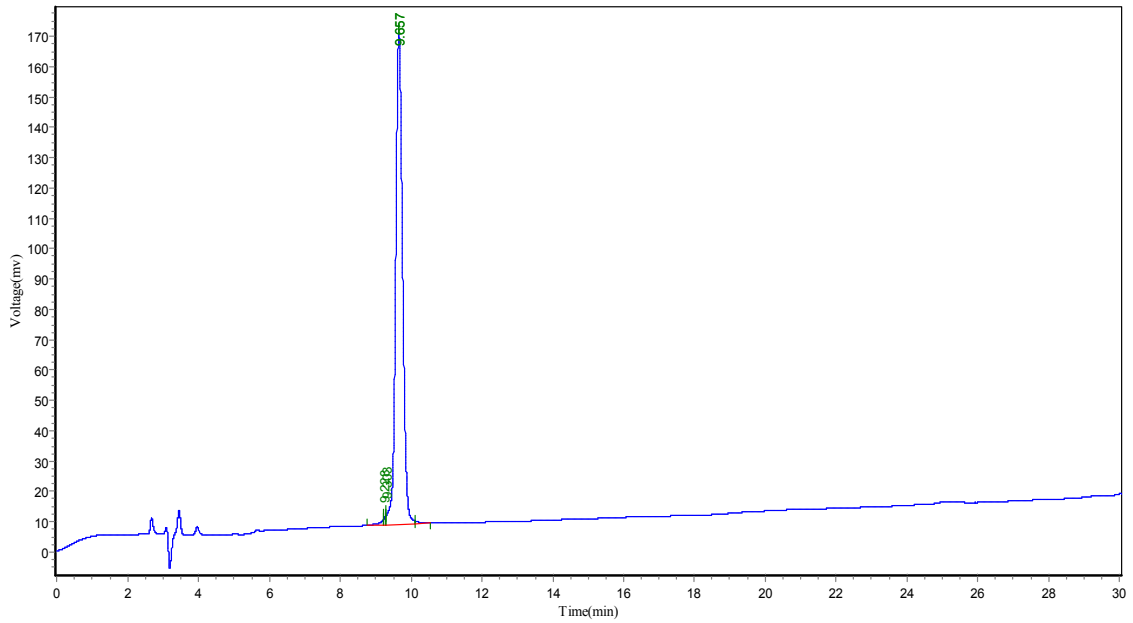

Peak No.	Ret Time	Height	Area	Conc.
1	9.228	1919.429	13962.481	0.6299
2	9.303	3083.886	11409.248	0.5147
3	9.657	161727.922	2183605.500	98.5147
4	9.657	1089.382	7550.142	0.3406
Total				100