


# GHRP-2 MS TEST REPORT

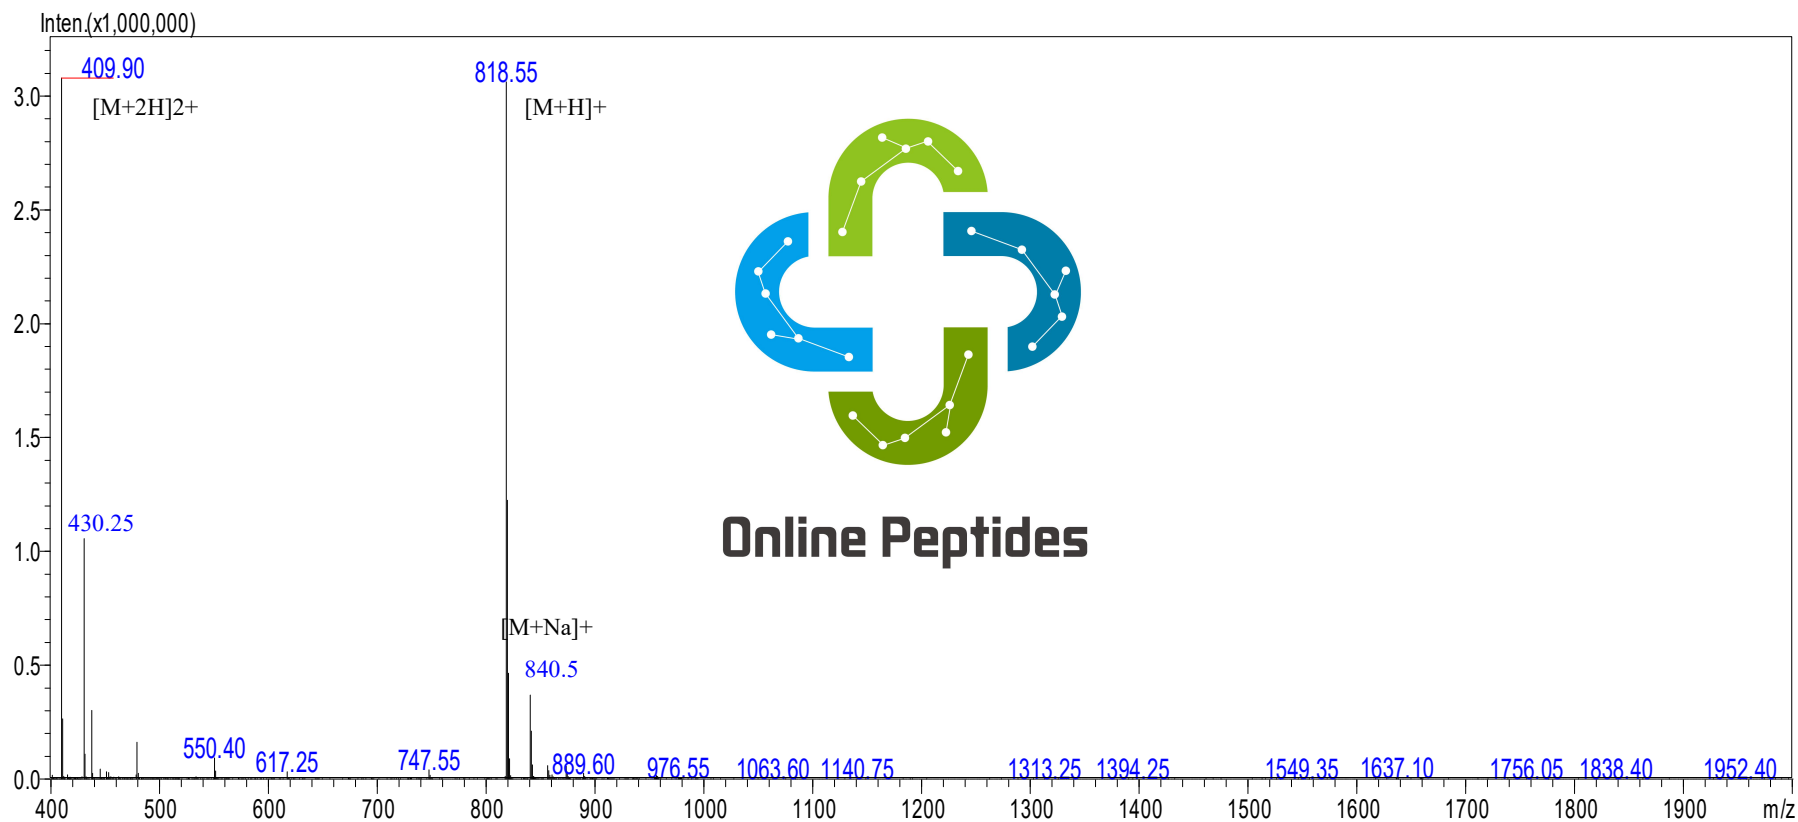

Date and Time: 2017-9-16 10:41:30  
Sample : GHRP-2  
MW : 818.0  
Lot No. : P170916G2

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H<sub>2</sub>O/50%ACN