


GHRP-6 MS TEST REPORT

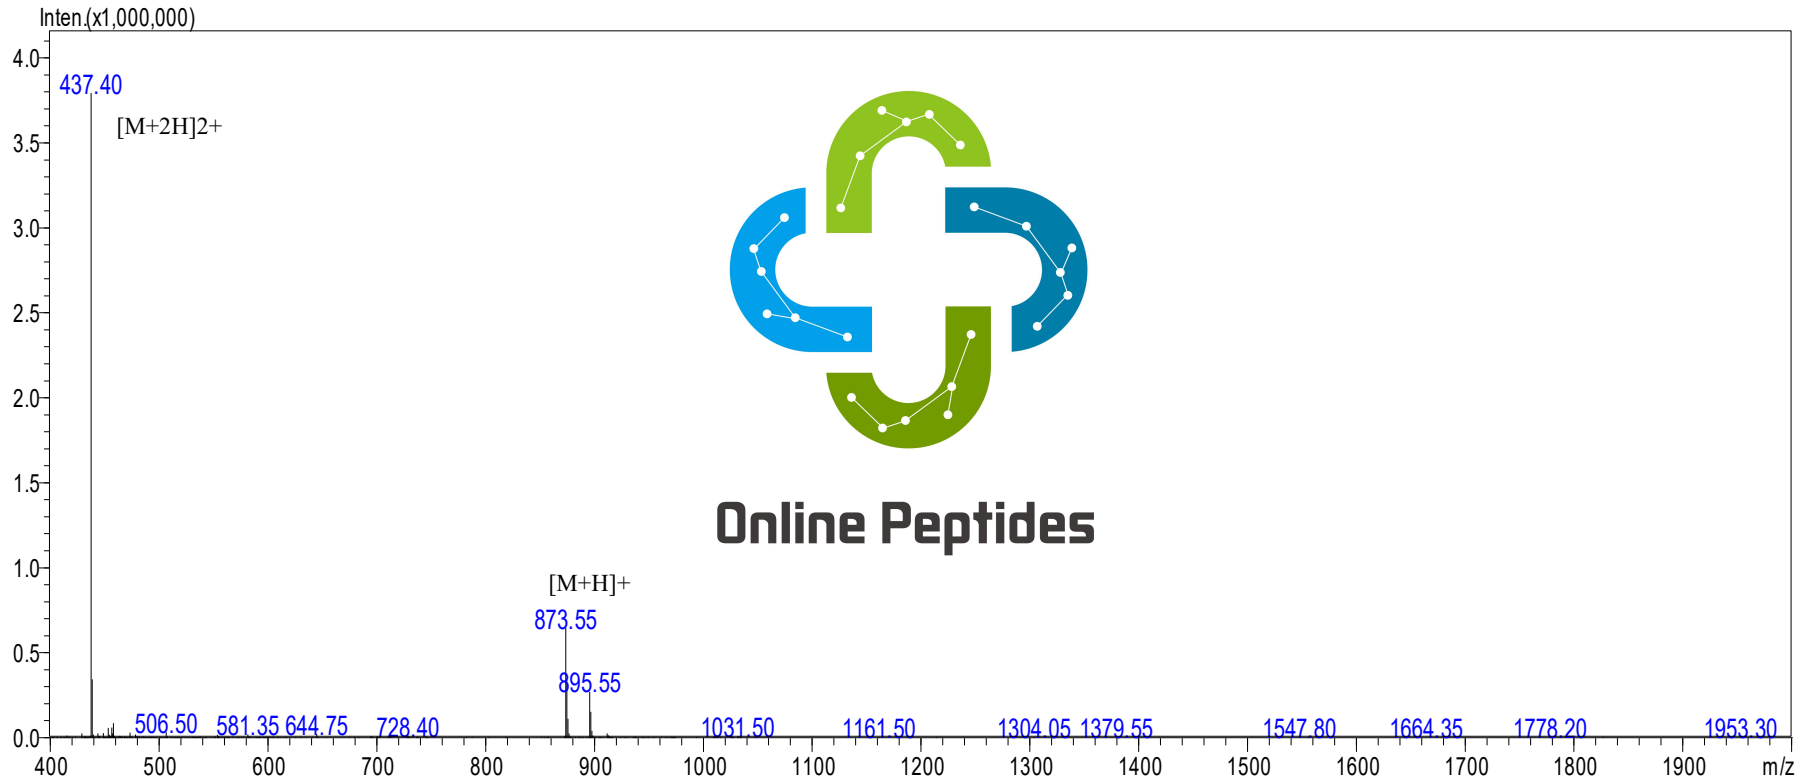

Date and Time: 2017-6-6 14:21:42
Sample : GHRP-6
MW : 873.04
Lot No. : P170606G6

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H₂O/50%ACN